

A High-Speed Spatial (Linear) Scanning Pyrometer: A Tool for Diagnostics, Temperature Mapping, and Property Determinations at High Temperatures

A. Cezairliyan, R.F. Chang, and G.M. Foley
Thermophysics Division
National Institute of Standards and Technology
Gaithersburg, Maryland 20899

Development of a fast spatial scanning pyrometer for temperature measurements above 1500 K is described.

The salient features of the pyrometer are:

1. it measures spectral radiance temperature (at $0.65\ \mu\text{m}$) at 1024 points along a straight line (25 mm long) on the target,
2. it has no moving parts and uses a self-scanning linear array of silicon photodiodes as the detector,
3. its output is recorded digitally every $1\ \mu\text{s}$ with a full-scale resolution of about 1 part in 4000, permitting performance of a complete cycle of measurements (1024 points) in about 1 ms.

Operational characteristics of the pyrometer are given. Examples of measurements of the temperature along rapidly heated (resistive self-heating) specimens (rod, tube, strip) are presented. Potential use of the pyrometer in experiments, both ground-based and in microgravity, requiring temperature mapping and property determinations of the specimen at high temperatures is discussed.

A HIGH-SPEED SPATIAL (LINEAR) SCANNING PYROMETER:
A TOOL FOR DIAGNOSTICS, TEMPERATURE MAPPING, AND
PROPERTY DETERMINATIONS AT HIGH TEMPERATURES

A. Cezairliyan, R.F. Chang, and G.M. Foley
Thermophysics Division
National Institute of Standards and Technology
Gaithersburg, Maryland 20899

Abstract

Development of a fast spatial scanning pyrometer for temperature measurements above 1500 K is described.

The salient features of the pyrometer are:

1. it measures spectral radiance temperature (at $0.65\ \mu\text{m}$) at 1024 points along a straight line (25 mm long) on the target,
2. it has no moving parts and uses a self-scanning linear array of silicon photodiodes as the detector,
3. its output is recorded digitally every $1\ \mu\text{s}$ with a full-scale resolution of about 1 part in 4000, permitting performance of a complete cycle of measurements (1024 points) in about 1 ms.

Operational characteristics of the pyrometer are given. Examples of measurements of the temperature along rapidly heated (resistive self-heating) specimens (rod, tube, strip) are presented. Potential use of the pyrometer in experiments, both ground-based and in microgravity, requiring temperature mapping and property determinations of the specimen at high temperatures is discussed.

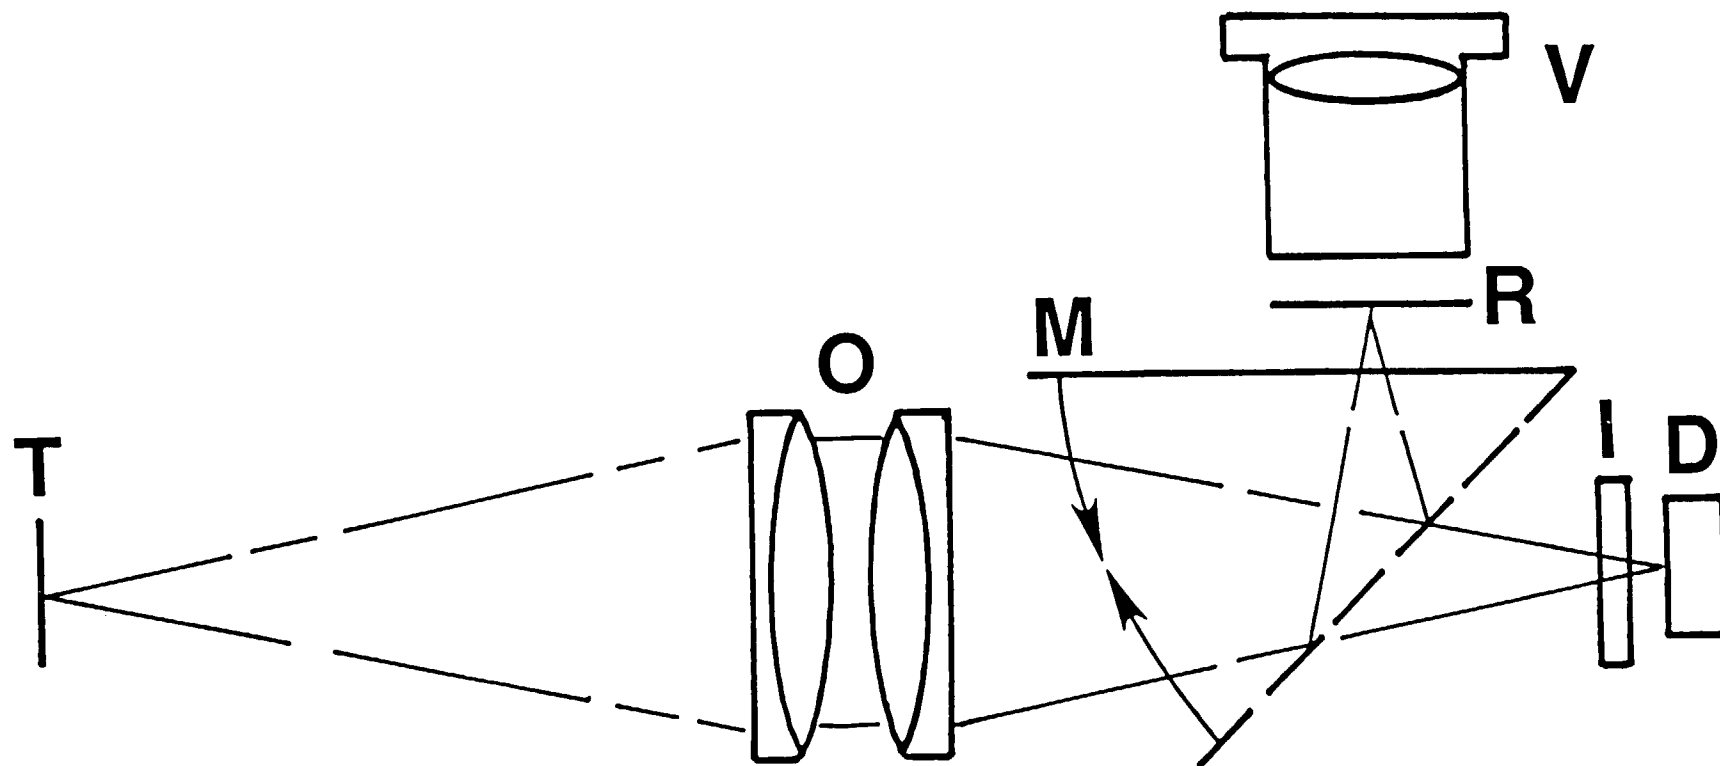


Fig. 1. Schematic diagram of the spatial (linear) scanning pyrometer where T is the target, O is the objective lens (1:1 magnification), I is the interference filter (40 nm bandwidth centered at 650 nm), D is a 1024-element silicon photodiode linear array, V is the viewing eyepiece, R is a reticle and M is a movable mirror.

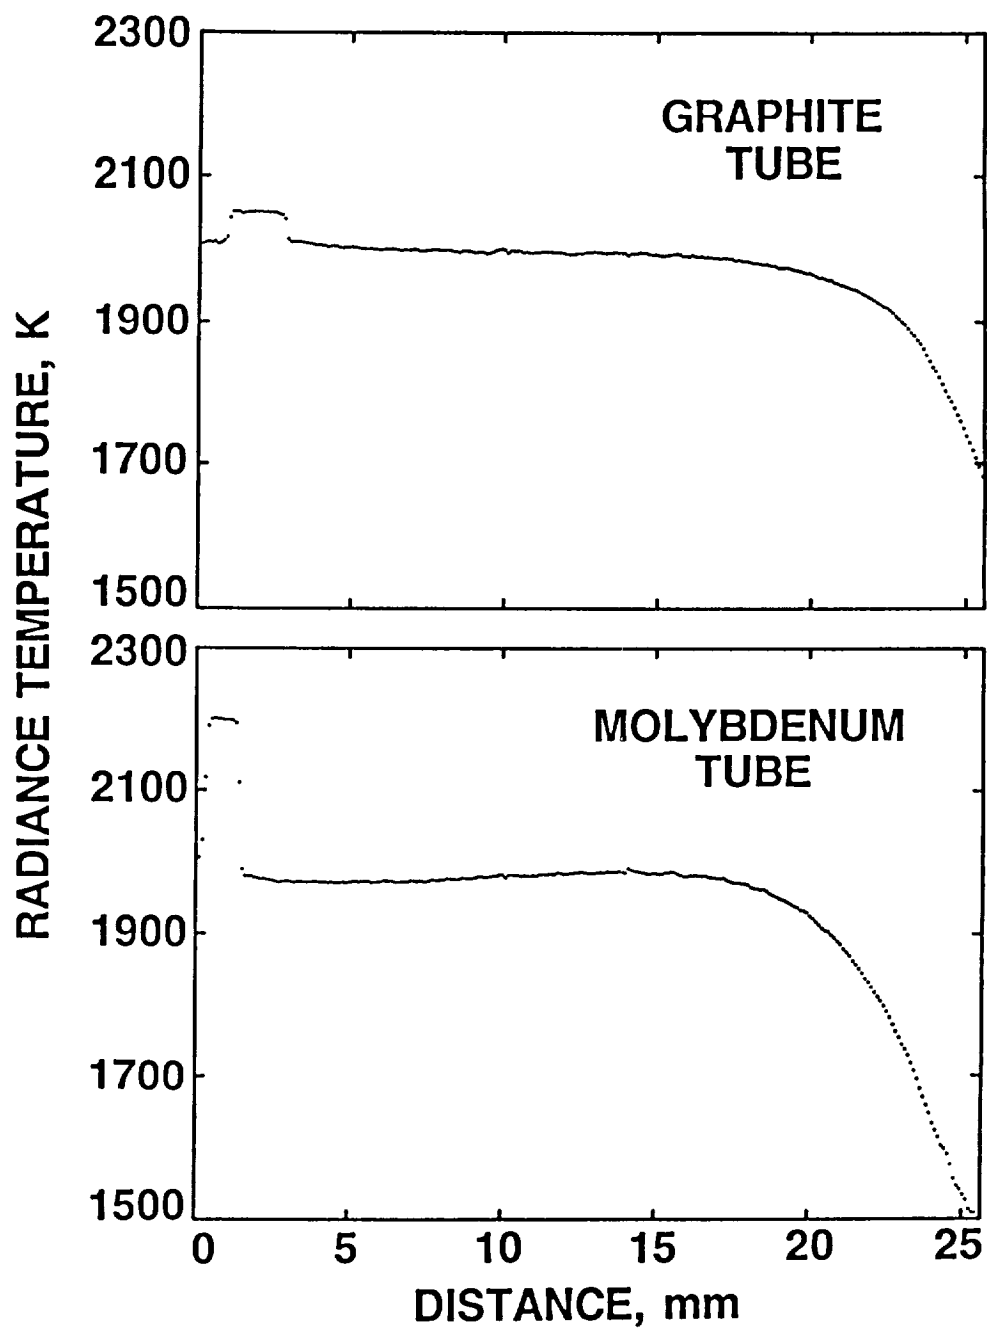


Fig. 2. A profile of the radiance temperature as measured by the pyrometer in a (1 ms) scan along one-half of a graphite tube (upper) and a molybdenum tube (lower) during rapid pulse heating. The region of increased radiance (left) is due to a small "blackbody" hole fabricated through the wall near the middle of the tube. A large temperature gradient (right) is observed along the specimen near the water-cooled clamp.

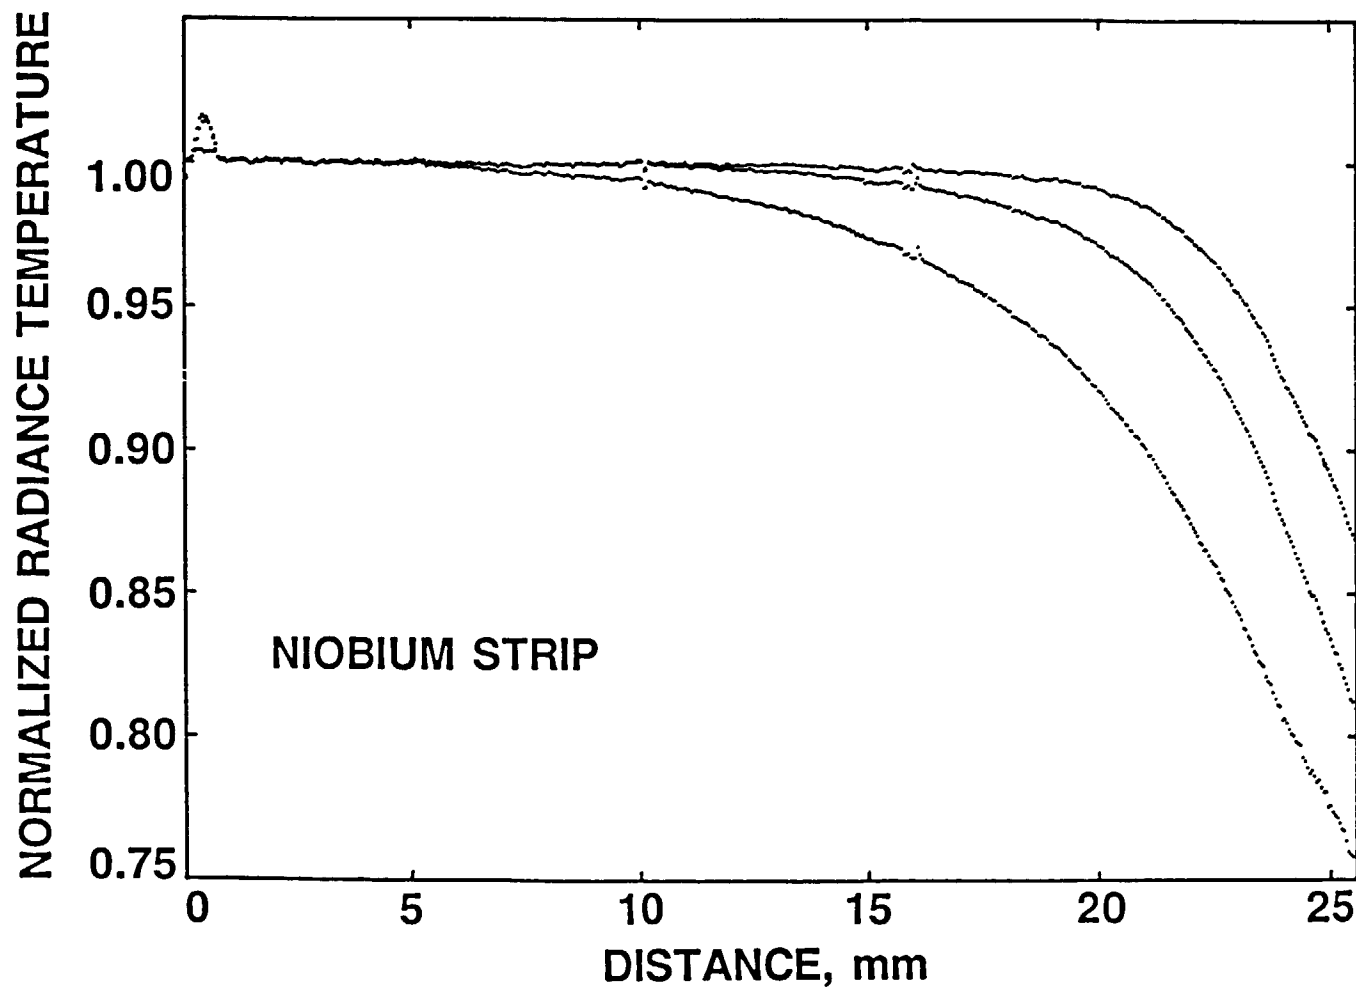


Fig. 3. Profiles of the radiance temperature as measured by the pyrometer in 1 ms-scans along one-half of a niobium strip during pulse heating at three different rates: highest heating rate (uppermost profile), lowest heating rate (lowermost profile).